


Provided for non-commercial research and education use.
Not for reproduction, distribution or commercial use.

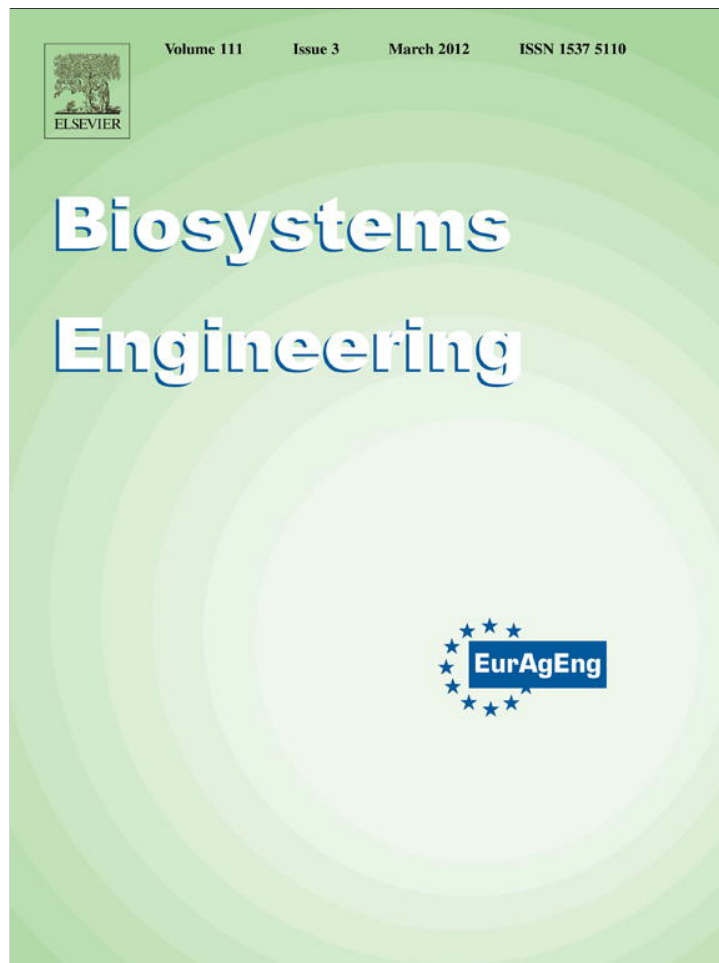

This article appeared in a journal published by Elsevier. The attached copy is furnished to the author for internal non-commercial research and education use, including for instruction at the authors institution and sharing with colleagues.

Other uses, including reproduction and distribution, or selling or licensing copies, or posting to personal, institutional or third party websites are prohibited.

In most cases authors are permitted to post their version of the article (e.g. in Word or Tex form) to their personal website or institutional repository. Authors requiring further information regarding Elsevier's archiving and manuscript policies are encouraged to visit:

<http://www.elsevier.com/copyright>

Available online at www.sciencedirect.com

SciVerse ScienceDirect

journal homepage: www.elsevier.com/locate/issn/15375110

Research Paper

Evaluating the storage environment in hypobaric chambers used for disinfesting fresh fruits

Shunshan Jiao^b, Judy A. Johnson^c, John K. Fellman^d, Dennis S. Mattinson^d,
Juming Tang^b, Tom L. Davenport^e, Shaojin Wang^{a,b,*}

^a Northwest A&F University, College of Mechanical and Electronic Engineering, Yangling, Shaanxi 712100, China

^b Department of Biological Systems Engineering, Washington State University, 208 L.J. Smith Hall, Pullman, WA 99164-6120, USA

^c USDA-ARS, San Joaquin Valley Agricultural Sciences Center, 9611 S. Riverbend Avenue, Parlier, CA 93648, USA

^d Department of Horticulture and Landscape Architecture, Washington State University, Pullman, WA 99164-6414, USA

^e Atlas Technologies, VivaFresh Div., 1452 North Krome Ave., Suite 101i, Florida City, FL 33034, USA

ARTICLE INFO

Article history:

Received 20 September 2011

Received in revised form

29 November 2011

Accepted 8 December 2011

Published online 11 January 2012

Low pressure (LP) treatment has potential as an alternative non-chemical postharvest disinfestation method for fresh fruits. A validated computer simulation model was used to determine the thickness of foam insulation needed to cover the hypobaric chamber walls in order to stabilise the air temperature within the hypobaric chambers that were housed in a cold storage room with fluctuating air temperatures. The stability of pressure, temperature and relative humidity levels in the LP system was evaluated together with various O₂ concentrations, evacuation, venting and leakage rates. Results showed that the added foam covering the chambers maintained the temperature variation of the hypobaric chamber wall to within ± 0.2 °C and inside air to within ± 0.1 °C. The regulating system kept pressure to within $\pm 1\%$ of the set point, and maintained relative humidity at nearly saturated levels ($>98\%$) under various air exchange rates and pressures, with a chamber leakage rate of 0.009 kPa h⁻¹ and LP system leakage rate of 0.480 kPa h⁻¹. Given that the hypobaric chamber displayed adequate performance characteristics, further studies will be conducted to evaluate LP treatment efficacy for fresh fruits.

© 2011 IAGrE. Published by Elsevier Ltd. All rights reserved.

1. Introduction

Because the process is completely organic, chemical free, and environmentally sustainable, low pressure (LP) has been considered as a non-chemical alternative to chemical fumigants for disinfestation of agriculture products. LP is achieved by evacuating air from a chamber holding the stored product to be treated to proportionally reduce the partial pressures of individual atmospheric gases, especially O₂. Most LP systems

targeting fresh fruits and vegetables utilise a method to maintain high humidity, thus water loss, commodity respiration, and production of the ripening hormone ethylene are reduced under LP conditions to prevent wilting and fruit ripening during storage (Burg, 2004). In addition, LP discourages commodity deterioration caused by bacterial and fungal decay and is capable of killing all life stages of many insects infesting agricultural commodities (Burg, 2004). Insect mortality increases with increasing storage time in LP, and is

* Corresponding author. Northwest A&F University, College of Mechanical and Electronic Engineering, Yangling, Shaanxi 712100, China. Tel.: +86 29 87092391; fax: +86 29 87091737.

E-mail addresses: shaojinwang@nwsuaf.edu.cn, shaojin_wang@wsu.edu (S. Wang).

1537-5110/\$ – see front matter © 2011 IAGrE. Published by Elsevier Ltd. All rights reserved.

doi:10.1016/j.biosystemseng.2011.12.003

Nomenclature			
A	surface area, m ²	T	temperature, °C
C	O ₂ concentration, %	V	volume, m ³
C _a	ambient O ₂ concentration, %	x, y	distances (m) along the axial direction, m
C _{O₂}	final O ₂ concentration, %	α	thermal diffusivity, m ² s ⁻¹
C _p	specific heat, J kg ⁻¹ °C ⁻¹	ρ	density, kg m ⁻³
h ₁	external surface heat transfer coefficients, W m ⁻² °C ⁻¹	<i>Subscripts</i>	
h ₂	internal surface heat transfer coefficients, W m ⁻² °C ⁻¹	a	interior air
k	thermal conductivity, W m ⁻¹ °C ⁻¹	c	chamber wall
l	material thickness, m	d	dry-bulb
P	pressure, kPa	f	foam
P ₀	ambient air pressure at sea level, kPa	set	total inside the hypobaric chamber
RH	relative humidity, %	sv	saturated vapour
t	time, s	o	outside air
		v	vapour
		w	wet-bulb
		0	reference

strongly temperature and humidity dependant (Johnson, 2010; Mbata, Phillips, & Payton, 2004). In order to develop a disinfection treatment for fresh fruits using LP, its impact on insect mortality must be evaluated. However, it is essential to firstly evaluate the stability of the storage environment in hypobaric chambers before conducting future efficacy tests.

The effect of low pressure on insects has been investigated since the 1880s (Back & Cotton, 1925). Attempts to use LP for disinfecting a variety of agricultural commodities began with Back and Cotton (1925), followed by studies by Bare (1948), Calderon, Navarro, and Donahaye (1966), and Calderon and Navarro (1968). More recently, the need to find non-chemical treatments to kill quarantine insects in transhipped loads of imported and exported commodities has increased interest in the use of LP technology for disinfection (Burg, 2010; Chen, White, & Robinson, 2005; Davenport, Burg, & White, 2006; Johnson & Zettler, 2009; Mbata & Philips, 2001; Navarro et al., 2001, 2007). LP storage provides the added benefit of preserving the fresh-picked quality of fully mature fruits and vegetables for months (Burg & Burg, 1966; Davenport et al., 2006; Knee & Aggarwal, 2000; Li, Zhang, & Wang, 2008). For example, Challot and Vincent (1977) used a treatment of 80.0 kPa to preserve cacao bean quality in polyethylene bags. Li and Zhang (2006) achieved an extension in shelf-life of green asparagus with a pressure of 15.0 ± 5.0 kPa.

Stability of pressure, temperature and relative humidity is an important performance characteristic of LP systems for fresh produce. Except for the influence of the vacuum pump, pressure stability mainly depends on chamber tightness, precision of the pressure sensor and regulator, and the air exchange system. The air exchange system is not only important in maintaining the desired relative humidity and pressure, but by allowing the continuous intake of fresh air and removal of metabolic gases produced by the fruit, it prevents the build-up of respiratory byproducts and ethylene within the hypobaric chamber. Since hypobaric chambers are generally located in temperature-controlled incubators, cold storage rooms or plant growth chambers (Chen et al., 2005; Davenport et al., 2006; Navarro et al., 2007), the temperature variations of the chamber walls and air inside the chambers

are largely influenced by the precision of the surrounding temperature-controlled environment. A large temperature variation results in condensation and evaporation cycles on the inner surface of chamber walls and product surfaces, which could cause unexpected water loss from products and even damage to product quality, especially in the water-saturated air necessary for storing fresh fruits. To avoid condensation and evaporation cycles, the surrounding air temperature variation should be maintained within ±0.5 °C (Davenport et al., 2006) and the hypobaric chamber wall temperature should remain within ±0.2 °C in the temperature range of -17 °C to 49 °C (Burg, 2004). A practical solution could be to use insulating foam around the chamber and humidifier to reduce air temperature variation, thus maintaining the saturated humidity in the hypobaric chamber.

It is difficult in most laboratory LP systems to achieve leak-free low pressures, and usually leaks are not evident because pressures are maintained at the set value using pressure regulators (Burg, 2004). Leakage is a major problem in lab-scale LP systems, resulting in higher than desired pressure and most importantly lower relative humidity which may cause more water loss of products. To avoid excess water loss in LP-treated products, the leakage rate should be kept below 0.6, 1.0, 1.5 and 5.0 kPa h⁻¹ at pressures of 1.3, 2.0, 2.7 and 5.3 kPa, respectively (Burg, 2004).

Insect mortality under LP is predominantly caused by low O₂ concentrations (Navarro & Calderon, 1979), although it has been reported that low relative humidity can also enhance the lethal effect of LP on insects (Johnson, 2010; Navarro, 1974, p. 118). When insects are placed into a hypoxic environment for a sufficient duration, adenosine triphosphate production is reduced, resulting in increasing membrane phospholipid hydrolysis (Herreid, 1980). Cell and mitochondrial membranes then become permeable, causing cell damage or death (Freidlander & Navarro, 1983; Mitcham, Martin, & Zhou, 2006). Effective control of insects has been observed at O₂ concentrations less than 6.6%, and especially at 0.15%–0.30% (Burg, 2004). Thus, it is essential to estimate the level of O₂ concentration in hypobaric chambers as influenced by pressure, temperature and relative humidity.

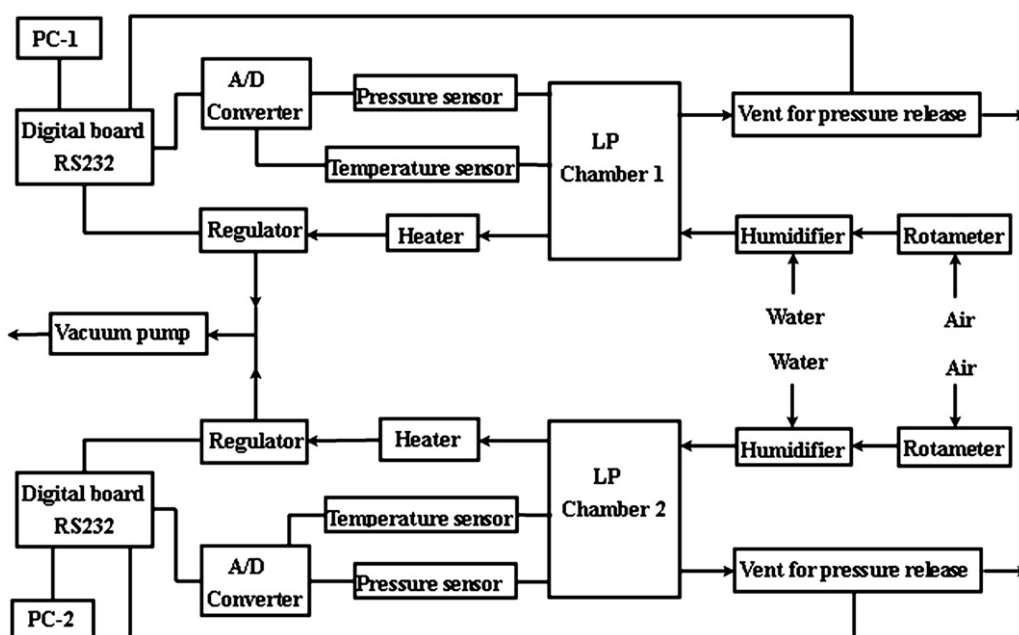


Fig. 1 – Diagram of the low pressure (LP) system, including vacuum, air exchange, pressure release and measurement systems (lines with an arrow indicate the gas flow through plastic soft pipe and those without an arrow indicate signal transmission via wire).

The objectives of this research were firstly to reduce the variations of air temperature in a hypobaric chamber housed in a cold storage room by using a validated energy balance model, and to evaluate the stability of pressure, temperature, and relative humidity in the chambers. Secondly, to determine O_2 concentrations as influenced by pressure, temperature, and relative humidity in the chambers. Finally, to determine the leakage rate of ambient air into the LP system.

2. Materials and methods

2.1. LP system

Two laboratory scale, VivaFresh™ (Model RDC-0005, Atlas Technologies, Port Townsend, WA, USA) LP systems using identical aluminium chambers ($0.61 \text{ L} \times 0.43 \text{ W} \times 0.58 \text{ H m}^3$) were used in the present study. Low pressure was achieved with a two-stage rotary vacuum pump (Model RV5, Edwards, Tewksbury, MA, USA) regulated by a compact proportional solenoid valve (Model PVQ33, SMC Co., Tokyo, Japan) controlled by a proportional/integral/derivative (PID) computer control system. Chamber pressure was monitored with a digital pressure gauge (Model HPS902, MKS Vacuum Technology, Boulder, CO, USA). A rotameter (Model FL-3841G, OMEGA Engineering Inc., Stamford, CT, USA) was used to adjust the air exchange rate, and the ingoing rarefied air was passed through a humidifier (Atlas Technologies, Port Townsend, WA, USA) before entering the hypobaric chamber in order to keep the relative humidity near saturation (100%). The relative humidity was calculated by measuring wet-bulb and dry-bulb temperatures using calibrated YSI 55000 Series GEM thermistors (Therm-x of California, Hayward, CA, USA)

having relatively high accuracy ($\pm 0.1\%$) (Wang, Tang, & Younce, 2003). Similar thermistors were used to measure the temperatures inside the chamber and the exterior chamber wall. All data from temperature and pressure sensors in the LP system were digitised and sent to a computer control and recording system via an RS-232 serial port. The diagram of the system is shown in Fig. 1.

2.2. Model development

Based on preliminary tests, air temperature variation in the cold storage room was $\pm 1.1 \text{ }^\circ\text{C}$, which exceeded the required surrounding air temperature variation ($\pm 0.5 \text{ }^\circ\text{C}$) for hypobaric chambers (Davenport et al., 2006). To reduce the influence of air temperature variations from the cold storage room, polyurethane foam insulation was used to completely cover the hypobaric chambers. A heat transfer model was developed and validated to determine an adequate thickness of foam insulation.

The computer simulation model consisted of energy balance equations for the interior air, the chamber wall, and the foam insulation (Fig. 2). It included convective heat transfer from the cold room air to the foam, conductive heat transfer through the foam and the chamber wall, and convective heat transfer from the chamber wall to the interior air. For heat conduction in the rectangular-shaped objects, the following governing equation was used:

$$\frac{1}{\alpha} \frac{\partial T}{\partial t} = \left(\frac{\partial^2 T}{\partial x^2} + \frac{\partial^2 T}{\partial y^2} \right) \quad (1)$$

where α is thermal diffusivity ($\text{m}^2 \text{ s}^{-1}$), T is the temperature ($^\circ\text{C}$), t is time (s), x and y are the distances (m) along the axial direction. Thermal diffusivity (α) is derived from $k/\rho C_p$, where

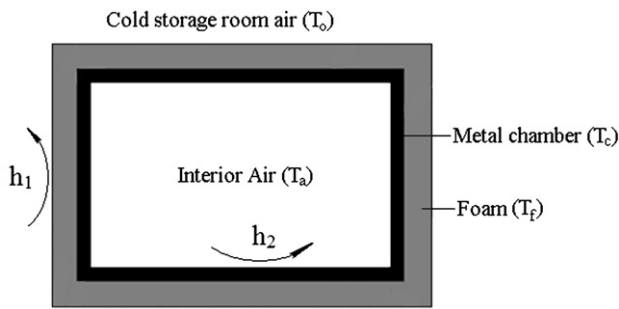


Fig. 2 – Diagram of the heat transfer model in an insulated metal chamber in a cold storage room (h_1 – external surface air convection coefficient, h_2 – internal surface air convection coefficient).

k is the thermal conductivity ($\text{W m}^{-1}\text{C}^{-1}$), ρ is the density (kg m^{-3}), and C_p is the specific heat ($\text{J kg}^{-1}\text{C}^{-1}$). The boundary conditions were represented by the following heat exchange equation describing convection from the ambient medium (air) and the foam surface (f):

$$\begin{matrix} -k \frac{\partial T_f}{\partial l} \Big|_{l=l_o} & = & h_1 [T_f(t) - T_o] \\ \text{Heat exchange flow} & & \text{Heat exchange flow} \\ \text{at foam surface} & & \text{from the exterior} \end{matrix} \quad (2)$$

where l is the material thickness (m), h_1 is the external surface heat transfer coefficients ($\text{W m}^{-2}\text{C}^{-1}$) and T_f is the temperature of the foam ($^{\circ}\text{C}$).

The energy balances for the interior air, chamber and foam were described below:

$$\rho_a C_a V_a \frac{dT_a}{dt} = h_2 A_a (T_c - T_a) \quad (3)$$

$$\rho_c C_c V_c \frac{dT_c}{dt} = \frac{K_c}{l_c} A_c (T_f - T_c) - h_2 A_c (T_c - T_a) \quad (4)$$

$$\rho_f C_f V_f \frac{dT_f}{dt} = h_1 A_f (T_o - T_f) - \frac{K_f}{l_f} A_f (T_f - T_c) \quad (5)$$

where A is the surface area (m^2), V is the volume (m^3), subscripts a, c, f and o represent interior air, chamber wall, foam, and outside air, respectively; h_1 and h_2 are the external and internal surface heat transfer coefficients ($\text{W m}^{-2}\text{C}^{-1}$), respectively. Forced and natural convections for the external and internal heat convections were considered. The values of

h_1 and h_2 were selected to be 50 and $10 \text{ W m}^{-2}\text{C}^{-1}$ based on the literature (Chung, Wang, & Tang, 2007). The properties of the various materials in the system were shown in Table 1 and the thickness of the aluminium chamber wall was 0.006 m. The partial differential Eqs. (3)–(5) were reduced to algebraic equations using the finite difference method. Each material was assumed to have a homogenous and uniform temperature distribution. Temperatures of each material were calculated at a time interval of 1 s using the Gauss-Seidel numerical method coded in Quick Basic (v4.5, Microsoft Co., WA, USA) software.

2.3. Model validation and application

To validate the proposed heat transfer model, a stainless steel rectangular box with the interior dimension of $0.29 \text{ L} \times 0.15 \text{ W} \times 0.045 \text{ H m}^3$ and with chamber wall thickness of 0.001 m was placed in a cold storage room, and the box was wrapped with insulation foam using a thickness of 0.013 m. Two type-T thermocouples connected to a data logger (DL2e, Delta-T Devices Ltd., Cambridge, U.K.) were used to measure the air temperatures in the cold storage room and the box. The measured air temperature of the cold storage room was used as input for the model, while the resulting calculated air temperature for the box interior was compared with the measured data to validate the simulation model. The validated model was used to predict the influence of foam thickness on the hypobaric chamber wall and inside air temperature variations. Foam thickness ranging from 0.001 m to 0.03 m was considered and the corresponding hypobaric chamber wall and inside air temperature variations were simulated. The thickness of foam insulation which can reduce the temperature variation of the hypobaric chamber wall to within $\pm 0.2^{\circ}\text{C}$ would be used for subsequent studies.

2.4. Stability of pressure and temperature in the hypobaric chambers

After the hypobaric chambers were covered with the optimal thickness of foam insulation derived from the above model, the pressure and temperature stability within the two hypobaric chambers was determined at 4°C and 1.3, 3.3 and 6.7 kPa with air exchange rates of 0–2.0, 0–0.5, 0–0.2 volumes h^{-1} , respectively. The pressure was reduced to the set-point by the fully open vacuum pump, then held for more than 24 h, and finally released by opening the release valve. The evacuation or venting rates were estimated by dividing the difference

Table 1 – Thermal properties of different materials used in the current model simulation.

Materials	Density ρ (kg m^{-3})	Specific heat C_p ($\text{J kg}^{-1}\text{C}^{-1}$)	Thermal conductivity k ($\text{W m}^{-1}\text{C}^{-1}$)	Thermal diffusivity α ($\text{m}^2 \text{s}^{-1}$) $\times 10^{-7}$
Air ^a	1.2	1010	0.02	168
Foam ^a	32	1300	0.03	7.2
Stainless steel ^a	7900	477	14.9	39.5
Aluminium 6061 alloy ^b	2710	1256	167	491

a Data collected from Çengel. (2006).

b http://www.engineersedge.com/properties_of_metals.htm.

Table 2 – Environmental parameters measured in the hypobaric chamber held at 4 °C under different pressures and air exchange rates (mean ± SD).

Pressure set point (kPa)	Air exchange rate (volumes h ⁻¹)	Measured pressure (kPa)	Relative humidity (%)	Evacuation rate (kPa min ⁻¹)	Venting rate (kPa min ⁻¹)
1.3	0	1.336 ± 0.005	99.20 ± 1.13	2.733 ± 0.027	14.972 ± 0.080
	1	1.341 ± 0.007	99.30 ± 0.85	2.546 ± 0.240	14.745 ± 0.400
	2	1.343 ± 0.007	99.00 ± 1.41	2.386 ± 0.120	15.185 ± 0.240
3.3	0	3.329 ± 0.008	99.20 ± 1.13	4.573 ± 0.067	15.452 ± 0.560
	0.2	3.326 ± 0.011	98.40 ± 1.14	4.906 ± 0.027	14.919 ± 0.120
	0.5	3.330 ± 0.011	98.80 ± 0.85	4.666 ± 0.173	14.652 ± 0.773
6.7	0	6.631 ± 0.028	99.35 ± 0.78	6.439 ± 0.320	15.719 ± 2.160
	0.1	6.639 ± 0.029	99.10 ± 0.80	5.760 ± 0.267	14.359 ± 0.160
	0.2	6.638 ± 0.032	98.45 ± 0.78	5.920 ± 0.293	14.039 ± 0.027

between the ambient pressure and the set-point by the time needed to reach the set point or ambient pressure, the average values and standard deviations were calculated based on the two chambers.

2.5. O₂ concentration and relative humidity in the hypobaric chambers

Relative humidity (RH, %) was calculated using the measured dry-bulb and wet-bulb temperatures inside the hypobaric chamber according to the following equation (Lide, 1996):

$$RH(\%) = \frac{6.1078e^{17.269 \times T_w / (T_w + 237.3)} - 0.66 \times (T_d - T_w)}{6.1078e^{17.269 \times T_d / (T_d + 237.3)}} \times 100 \quad (6)$$

where T_w and T_d are the wet-bulb and dry-bulb temperature in °C, respectively.

The saturated vapour pressure (P_{sv} , kPa) is a function of the air temperature (T_a , °C) and can be calculated with the Antoine equation as follows:

$$P_{sv} = 0.133324 \times 10^{8.07131 - \frac{1730.63}{233.426 + T_d}} \quad (7)$$

The partial pressure of vapour is:

$$P_v = RH \times P_{sv} \quad (8)$$

Since the atmosphere in the hypobaric chamber can be considered as a mixture of gases, including water vapour, the

total pressure is the sum of the partial pressures of the components in the mixture based on Dalton's Law. The partial pressure of air (P_a , kPa) in the hypobaric chamber is:

$$P_a = P_{set} - P_v \quad (9)$$

where P_{set} is the total pressure inside the hypobaric chamber. According to the ideal gas law, the final O₂ concentration (C_{O_2} , %) is:

$$C_{O_2} = \frac{C_a \times P_a}{P_0} \quad (10)$$

where C_a is the ambient O₂ concentration (~21%), P_0 is the ambient air pressure at sea level, $P_0 = 101.3$ kPa.

According to Eqs. (9) and (10), O₂ concentration depends on the set-point pressure and the vapour pressure, which is a function of the air temperature and relative humidity in the chamber. The O₂ concentration was calculated at a temperature range of 0–20 °C, and three pressures of 1.3, 3.3 and 6.7 kPa. Relative humidity was derived from measurements taken under different temperatures and pressures (Table 2) and was considered to be 99%.

2.6. Determining LP system leakage rate

A reliable method to determine the leakage rate of LP systems is to reduce the pressure to a typical level, then turn off the

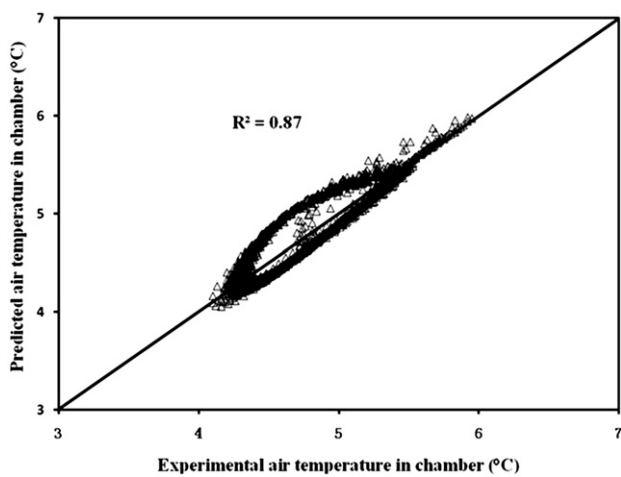


Fig. 3 – Comparison between predicted and experimental air temperatures in the chamber.

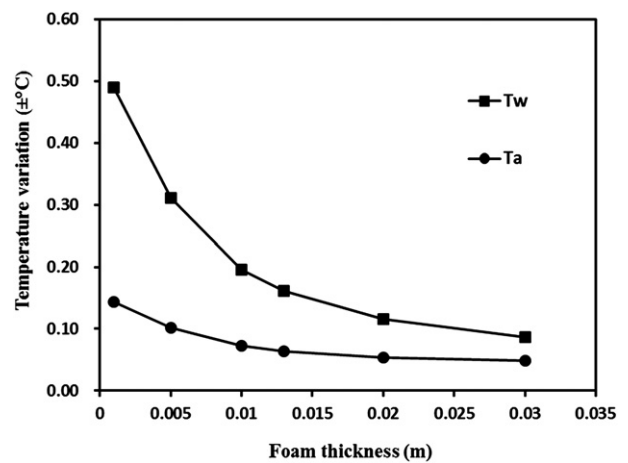


Fig. 4 – Simulated temperature variations for the hypobaric chamber wall (T_w) and inside air (T_a) under different insulation foam thicknesses.

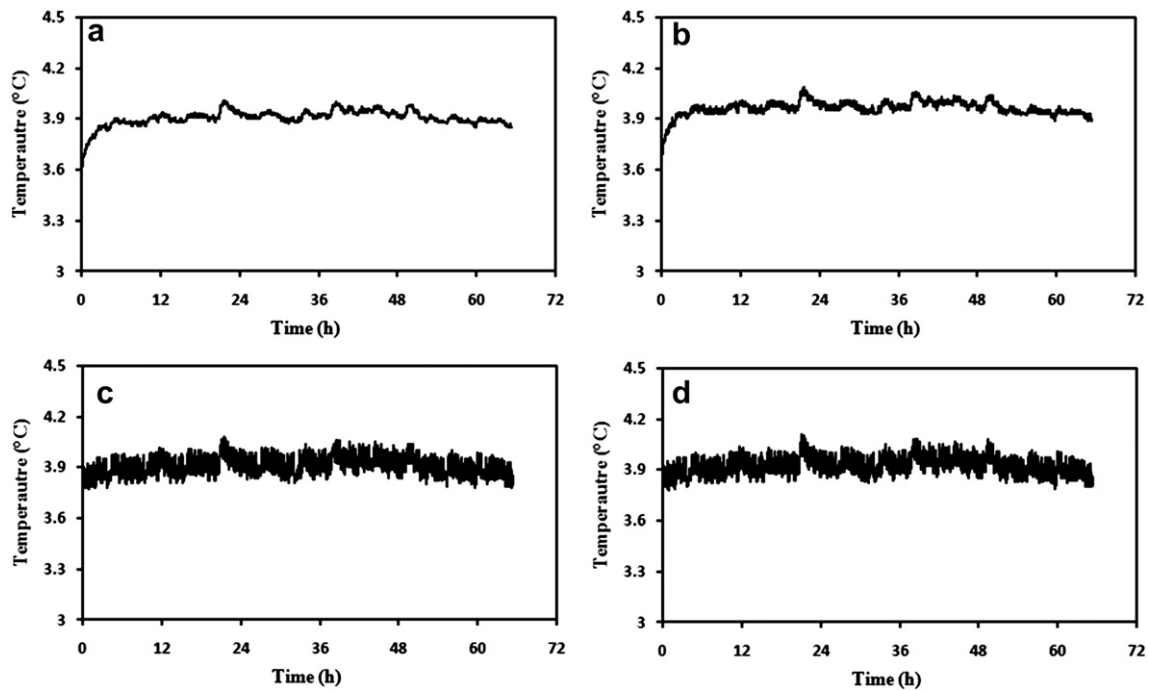


Fig. 5 – Temperature variation measured by four thermistor sensors at the set point temperature of 4 °C and 6.7 kPa pressure with 0.1 volumes h⁻¹ air exchange rate in one hypobaric chamber, (a) Wet-bulb temperature; (b) Dry-bulb temperature; (c) interior chamber wall temperature; (d) exterior chamber wall temperature.

vacuum pump, isolate the system, and finally measure the rate of pressure rise (Burg, 2004). In the current study, the pressure was first reduced to 1.3 kPa at 4 °C and then the rate of pressure increase was measured under three different conditions: (A) close off the vacuum system and the air exchange system, (B) close off the vacuum system but the air exchange system was set to 1.0 volumes h⁻¹, (C) open the vacuum system but shut down the air exchange system.

3. Results and discussion

3.1. Model validation and application

Figure 3 compares the air temperature data measured inside the small box to the temperatures predicted from the computer simulation heat transfer model over about 17 h. Since the proposed model fitted the experimental data well (coefficient of determination $R^2 = 0.87$), the established simulation model was used to predict the influence of the foam thickness on temperature variation inside the hypobaric chamber. Figure 4 shows the predicted variation of hypobaric chamber wall and inside air temperatures when the chamber was covered by different insulation foam thicknesses and housed in a 4 °C cold storage room. Temperature variation of the inside air was less than that of the hypobaric chamber wall, and both temperature variations decreased with increasing foam thickness. The results showed that the hypobaric chamber wall temperature variation could be reduced to within ± 0.2 °C and the inside air temperature could be maintained within ± 0.1 °C when the foam thickness was

> 0.01 m (Fig. 4). The results indicated that a layer of insulation foam at least 0.01 m thick can be used in the current study to maintain a relatively stable temperature of the hypobaric chamber walls. To ensure suitable stability in subsequent studies, commercially available polyurethane insulation foam (McMaster-Carr Supply Co., Los Angeles, CA, USA) 0.013 m thick was used.

3.2. Control stability of temperature and pressure

Figure 5 shows the variation of wet-bulb, dry-bulb, interior chamber wall and exterior chamber wall temperatures versus time at the set temperature of 4 °C for the cold storage room.

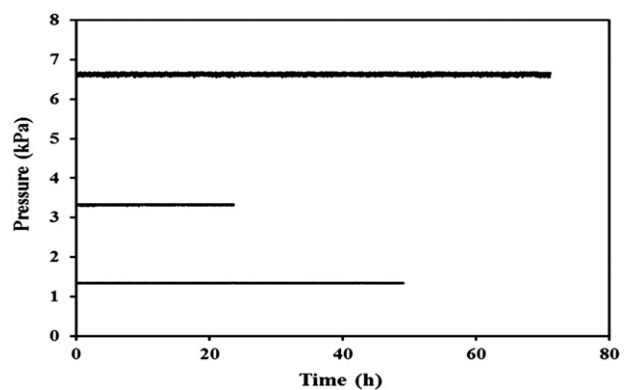


Fig. 6 – Stability of different pressures (1.3, 3.3, and 6.7 kPa) in the hypobaric chamber at 4 °C with the air exchange rate of 1, 0.2, and 0.1 volumes h⁻¹, respectively.

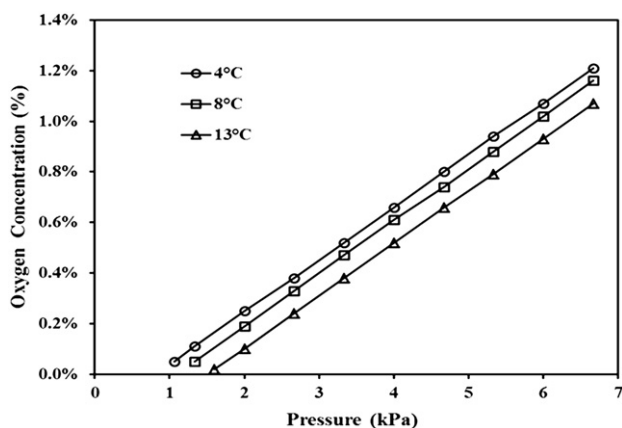


Fig. 7 – The estimated O₂ concentrations in the LP systems as a function of pressures at three different temperatures.

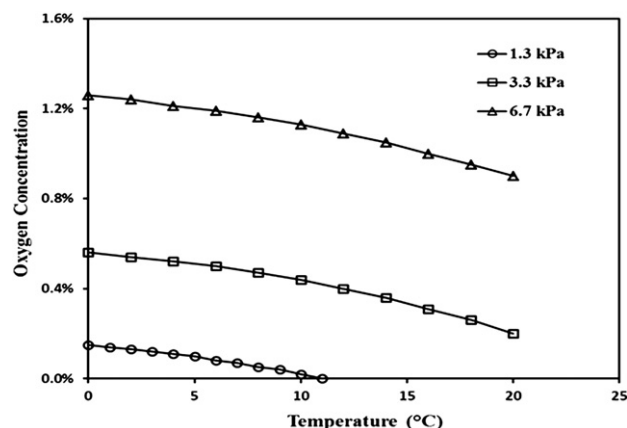


Fig. 8 – The O₂ concentration in LP systems as related to temperature at three different pressures.

The pressure was set to 6.7 kPa with 0.1 volumes h⁻¹ air exchange rate in one empty hypobaric chamber. The experimental variation of the inside air temperature was within ± 0.04 °C, which was a little smaller than the predicted value (± 0.06 °C), probably due to the slightly overestimated heat convection coefficient. With a temperature variation of ± 0.04 °C there were no condensation and evaporation cycles on the inner surface of hypobaric chamber walls, which was consistent with the literature (Burg, 2004). Addition of fruit stored at room temperature could cause temporary alteration in chamber temperature, but this should be of short duration and can be avoided by pre-cooling the fruit.

Figure 6 presents the pressure stability under different air exchange rates at 4 °C. The pressures were relatively stable at the set point with an accuracy of 1%, which is better than other systems mentioned in the literature (Chen et al., 2005; Davenport et al., 2006; Li & Zhang, 2006). Detailed statistical results were listed in Table 2 together with the evacuation and venting rates of the LP system. The pressure venting rate was much higher than the evacuation rate for all conditions (Table 2). The time for pressure to reduce from 93.3 kPa to all three tested pressures (1.3, 3.3, and 6.7 kPa) was 14–42 min, but the pressure venting time was less than 7 min for all of the tested pressures. These transient times during evacuating and venting are relatively short compared with the total LP treatment time, which usually takes several days for disinfestation. The evacuation and venting rates are constant parameters and are mainly dependent on the vacuum pump and air vents. Determining evacuation and venting rates will allow estimation of the time needed for increasing or decreasing pressure in the current LP system.

There were no clear differences under different air exchange rates (Table 2), since the flow rate was so small for the air exchange system compared with that of the vacuum pump or the vent for reducing or releasing pressure. The air exchange system is very important for maintaining fruit quality by removing metabolic gases generated by fruits (Burg, 2010) and keeping a relatively stable, low O₂ environment without ethylene. However, excessive air exchange rates have no benefits to the LP system, making the air difficult to saturate and causing a pressure drop in the pipe connected with the humidifier to the hypobaric chamber (Burg, 2004).

3.3. Relative humidity and O₂ concentration in the hypobaric chambers

Relative humidity, based on the measured wet-bulb and dry-bulb temperatures inside the hypobaric chamber at 4 °C under the different pressures and air exchange rates, is listed in Table 2. The humidifier installed in the current LP system maintained relative humidity inside the chamber at nearly saturated levels (>98%) under different pressures and air exchange rates. This saturated environment inside the hypobaric chamber would benefit fruit quality by reducing water loss (Burg, 2004). Even through the high relative humidity in hypobaric environments may encourage fungal growth (Lougheed, Murr, & Bérard, 1978), near saturated humidity conditions have been found to inhibit mould growth on most plant commodities (Burg, 2004; van den Berg & Lentz, 1978).

Calculated O₂ concentrations are shown in Figs. 7 and 8 at a temperature range of 0–20 °C and at three pressures (1.3, 3.3 and 6.7 kPa). O₂ concentration proportionally increased with pressure at each temperature (Fig. 7). At the same pressure, the O₂ concentration decreased with increasing temperature

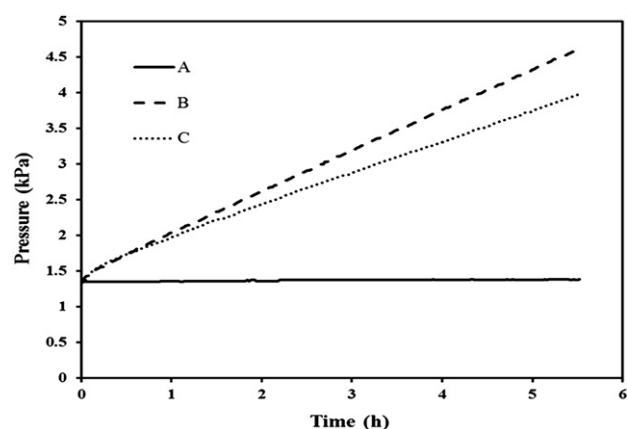


Fig. 9 – The leakage rates of hypobaric chamber under three different conditions at the temperature of 4 °C (A: Chamber only; B: With air exchange rate of 1 volumes h⁻¹; C: With vacuum system).

(Fig. 8). There was a limit for temperature reduction of O₂ concentration at each pressure level. For example, at 1.3 kPa O₂ concentrations reached 0% when the air temperature in the hypobaric chambers was increased to 11 °C (Fig. 8). O₂ concentrations were 0–0.2, 0.2–0.6, and 0.9–1.3% for 10, 25 and 6.7 kPa, respectively. Low O₂ concentration is the dominant mechanism for LP technology to control insects and <4.5% O₂ is necessary for effectively controlling the most susceptible stored-product insects (Navarro, 1978).

3.4. LP system leakage rate evaluation

Figure 9 shows the changes in hypobaric chamber pressure under three different conditions at 4 °C. The rate of increase in chamber pressure was 0.6 kPa h⁻¹ under an air exchange rate of 1 volumes h⁻¹; and was 0.5 kPa h⁻¹ when the air exchange system was shut down and the vacuum system was connected, and open, but the pump was turned off. When both the vacuum and air exchange systems were closed, the chamber pressure rose from 1.33 to 1.39 kPa in 5.5 h, indicating that the leakage rate was 0.01 kPa h⁻¹ for the hypobaric chamber. These chamber leakage rates were lower than those of the VacuFreshSM container reported by Burg (2004). Thus, the current hypobaric chambers would be expected to provide a useful system to further study the insect control and fruit quality preservation.

4. Conclusions

The good fit between the predicted results from the simulation and the experimental data suggests that the model could be useful in predicting temperature variability and the thickness of insulation needed for a variety of chambers. The model showed that insulation with a thickness of more than 0.01 m can reduce the temperature variation of hypobaric chamber wall to within ±0.2 °C and inside air to within ±0.1 °C. Experimental temperature data from the hypobaric chamber showed that with an insulation thickness of 0.013 m, temperature variation was well within the required levels, thereby avoiding condensation and evaporation cycles on the inner surface of the chamber walls. The LP system had the ability to control the pressure within 1% of the set point and maintained relative humidity at a nearly saturated level (>98%). O₂ concentration could be controlled at low levels (<0.6%) when the pressure was less than 3.3 kPa. These concentrations are well within the insecticidal range. The leakage rate of the hypobaric chamber was 0.01 kPa h⁻¹ and the whole LP system was 0.5 kPa h⁻¹ which was in the acceptable range. The good performance of the hypobaric chambers may provide a solid basis for future efficacy studies to develop non-chemical disinfestation treatments.

Acknowledgements

This research was supported by grant from USDA-NIFA-PMA (2010-343813-21619) and conducted at Washington State University Agricultural Research Centre. We sincerely thank

Atlas Technologies (Port Townsend, WA, USA) for providing the two hypobaric chamber systems and, R. Bothell, J. Bothell and T. Davenport for leasing, installing and tuning the LP system.

REFERENCES

- Back, E. A., & Cotton, R. T. (1925). The use of vacuum for insect control. *Journal of Agriculture Research*, 31, 1035–1041.
- Bare, C. O. (1948). The effect of prolonged exposure to high vacuum on stored tobacco insects. *Journal of Economic Entomology*, 41, 109–110.
- van den Berg, L., & Lentz, C. P. (1978). High-humidity storage of vegetables and fruits. *HortScience*, 13, 565–569.
- Burg, S. P. (2004). *Postharvest physiology and hypobaric storage of fresh produce*. Wallingford, UK: CABI.
- Burg, S. P. (2010). Experimental errors in hypobaric laboratory research. *Proceeding of 9th international controlled atmosphere research conference: Vol. 1* (pp. 45–61).
- Burg, S. P., & Burg, E. A. (1966). Fruit storage at subatmospheric pressures. *Science*, 153(3733), 314–315.
- Çengel, Y. A. (2006). *Heat and mass transfer: A practical approach* (3rd ed.). The McGraw Hill Companies. Appendix.
- Calderon, M., & Navarro, S. (1968). Sensitivity of three stored product insect species exposed to different low pressures. *Nature*, 218, 190.
- Calderon, M., Navarro, S., & Donahaye, E. (1966). The effect of low pressures on the mortality of six stored-product insect species. *Journal of Stored Products Research*, 2, 135–140.
- Challot, F., & Vincent, J. C. (1977). Storage of cocoa in vacuum in polyethylene containers. *Café Cocoa Thé*, 21(2), 129–136.
- Chen, Z. J., White, M. S., & Robinson, W. H. (2005). Low-pressure vacuum to control larvae of *hylotrupes bajulus* (Coleoptera: Cerambycidae). In C. Y. Lee, & W. H. Robinson (Eds.), *Proceedings of the fifth international conference on urban pests*. Malaysia: Perniagaan Ph'ng @ P&Y Design Network.
- Chung, H. J., Wang, S. J., & Tang, J. M. (2007). Influence of heat transfer with tube methods on measured thermal inactivation parameters for *Escherichia coli*. *Journal of Food Protection*, 70(4), 851–859.
- Davenport, T. L., Burg, S. P., & White, T. L. (2006). Optimal low-pressure conditions for long-term storage of fresh commodities kill Caribbean fruit fly eggs and larvae. *HortTechnology*, 16(1), 98–104.
- Freidlander, A., & Navarro, S. (1983). Effects of controlled atmospheres on the sorbitol pathway in *Ephestia cautella* pupae. *Experientia*, 39, 744–746.
- Herreid, C. F. (1980). Hypoxia in invertebrates. *Comparative Biochemistry and Physiology*, 67, 311–320.
- Johnson, J. A. (2010). Effect of relative humidity and product moisture on response of diapausing and nondiapausing Indianmeal moth (*Lepidoptera: Pyralidae*) larvae to low pressure treatments. *Journal of Economic Entomology*, 103, 612–618.
- Johnson, J. A., & Zettler, J. L. (2009). Response of postharvest tree nut lepidopteran pests to vacuum treatments. *Journal of Economic Entomology*, 102(5), 2003–2010.
- Knee, M., & Aggarwal, D. (2000). Evaluation of vacuum containers for consumer storage of fruits and vegetables. *Postharvest Biology and Technology*, 19, 55–60.
- Li, W. X., Zhang, M., & Wang, S. J. (2008). Effect of three-stage hypobaric storage on membrane lipid peroxidation and activities of defense enzyme in green asparagus. *LWT—Food Science and Technology*, 41, 2175–2181.
- Li, W. X., & Zhang, M. (2006). Effect of three-stage hypobaric storage on cell wall components, texture and cell structure of green asparagus. *Journal of Food Engineering*, 77, 112–118.

- Lide, D. R. (1996). CRC handbook of chemistry and physics. Section 15–32 (77th ed.). In *Determination of relative humidity from wet and dry bulb temperatures*, Boca Raton, FL: CRC Press.
- Lougheed, E. C., Murr, D. P., & Bérard, L. (1978). Low-pressure storage of horticultural crops. *HortScience*, 13, 21–27.
- Mbata, G. N., & Phillips, T. W. (2001). Effects of temperature and exposure time on mortality of stored-product insects exposed to low pressure. *Journal of Economic Entomology*, 94(5), 1302–1307.
- Mbata, G. N., Phillips, T. W., & Payton, M. (2004). Mortality of eggs of stored-product insects held under vacuum: effects of pressure, temperature, and exposure time. *Journal of Economic Entomology*, 97(2), 695–702.
- Mitcham, E. J., Martin, T., & Zhou, S. (2006). The mode of action of insecticidal controlled atmospheres. *Bulletin of Entomological Research*, 96, 213–222.
- Navarro, S. (1974). *Studies on the effect of alterations in pressure and composition of atmospheric gases on the tropical warehouse moth, Ephestia cautella (Wlk.), as a model for stored-products insects* (p. 118). Ph.D. thesis, Jerusalem: Hebrew University.
- Navarro, S. (1978). The effects of low oxygen tensions on three stored-product insect pests. *Phytoparasitica*, 6(2), 51–58.
- Navarro, S., & Calderon, M. (1979). Mode of action of low atmospheric pressures on *Ephestia cautella* (Wlk.) pupae. *Experientia*, 35, 620–621.
- Navarro, S., Donahaye, J. E., Dias, R., Azrieli, A., Rindner, M., Phillips, T., et al. (2001). Application of vacuum in a transportable system for insect control. In E. J. Donahaye, S. Navarro, & J. G. Leesch (Eds.), *Proc. int. conf. controlled atmosphere and fumigation in stored products*, Fresno, CA. 29 Oct–3 Nov. 2000 (pp. 307–315). Clovis, CA: Executive Printing Services.
- Navarro, S., Finkelman, S., Donahaye, J. E., Isikber, A., Rindner, M., & Dias, R. (2007). Development of a methyl bromide alternative for the control of stored product insects using a vacuum technology. In E. J. Donahaye, S. Navarro, C. Bell, D. Jayas, R. Noyes, & T. W. Phillips (Eds.), *Proc. int. conf. controlled atmosphere and fumigation in stored products*, Gold-Coast Australia. 8–13th August 2004 (pp. 227–234). Israel: FTIC Ltd. Publishing.
- Wang, S., Tang, J., & Younce, F. (2003). Temperature measurement. In D. R. Heldman (Ed.), *Encyclopedia of agricultural, food, and biological engineering* (pp. P987–P993). New York: Marcel Dekker.